



Certificate of Analysis


N-Acetyl Semax

Acetyl-L-Methionyl-L-alpha-glutamylhistidyl-L-phenylalanyl-L-prolylglycyl-L-proline

Compounds : N-AcSemax
Lot number : 2026-03-16
Analysis date : 2026-03-26
Purity % : 99.64%
Method : HPLC-UV-MS


Client : Bromantane, LLC
<http://Everychem.com/>

High Performance Liquid Chromatography (HPLC) UV – Purity Test

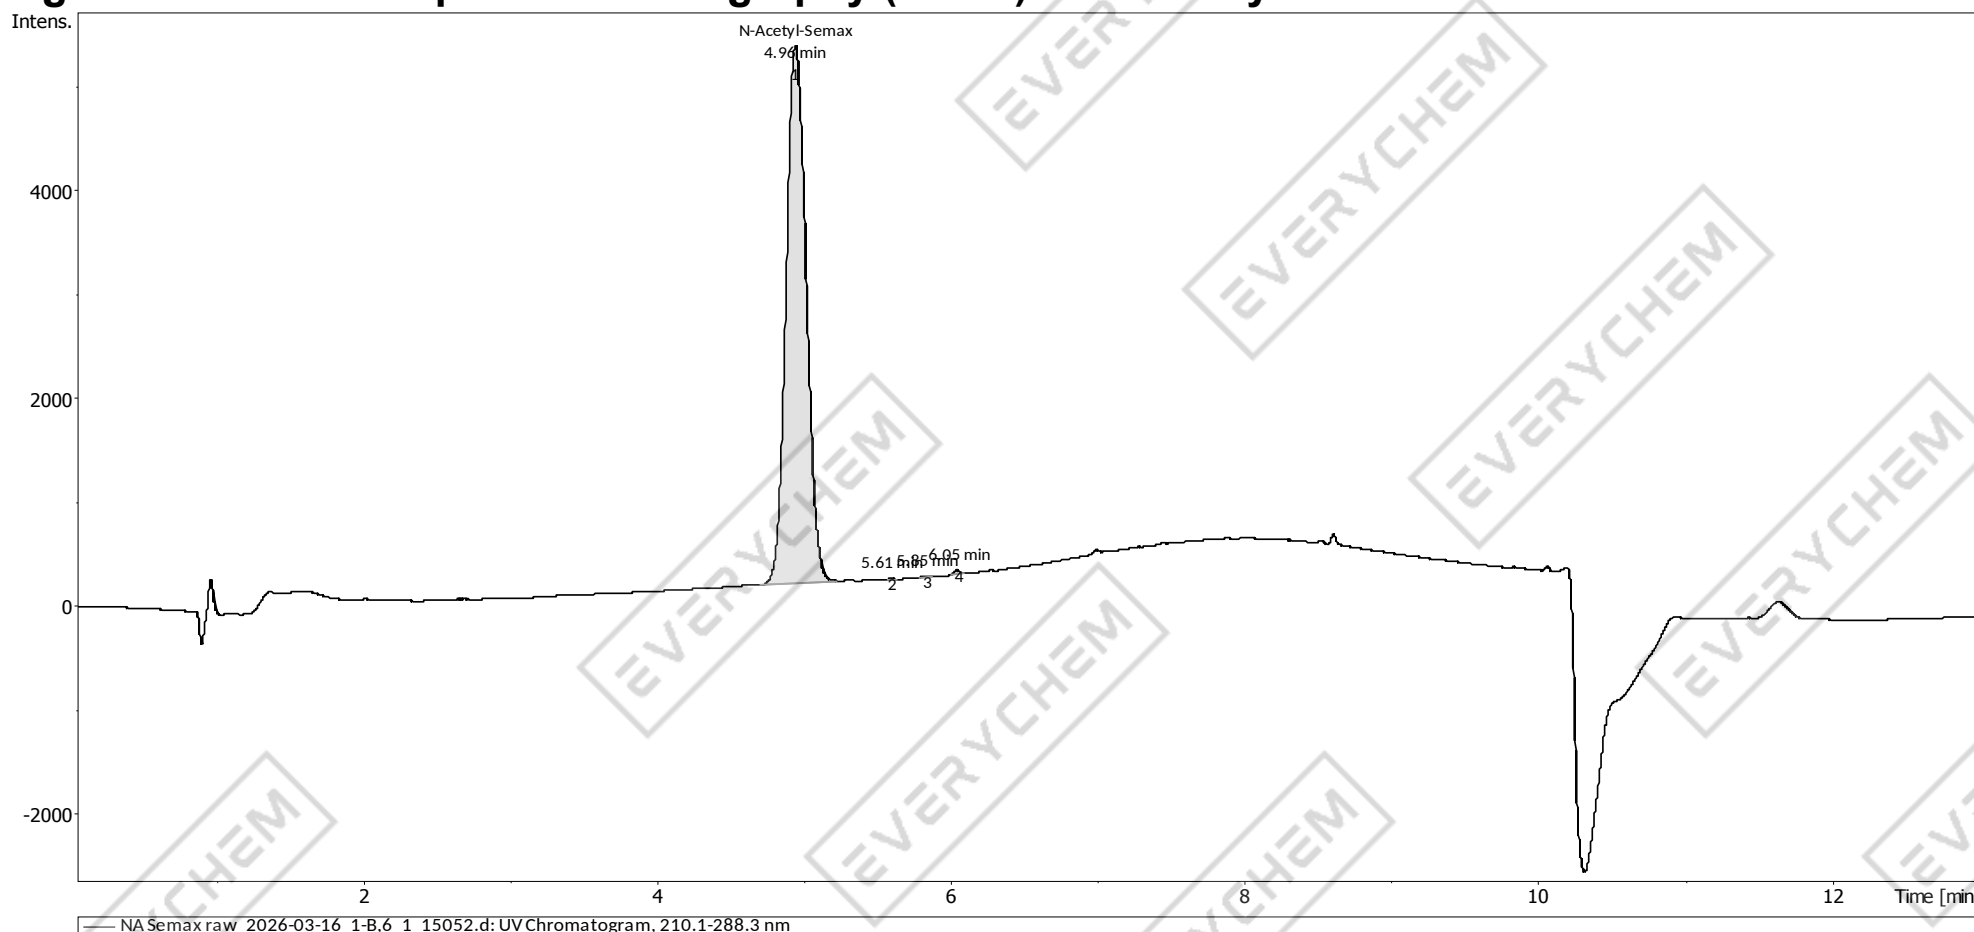

PEAK LIST				Number of detected peaks: 4	
	Time (min)	Area	%Area		
1	4.96	4.93E+04	99.64	N-AcSemax	
2	5.61	3.47E+01	0.07		
3	5.85	3.46E+01	0.07		
4	6.05	1.07E+02	0.22		

Analysis Performed by
 Ken Pendarvis, ChE
 Analytical Chemist
 MZ Biolabs
contact@mzbiolabs.com



2026-03-30

Note: Injectable peptides may contain salts and sugars to aid in solubility and act as pH buffers. These are not normally detected using UV and are not considered impurities.